
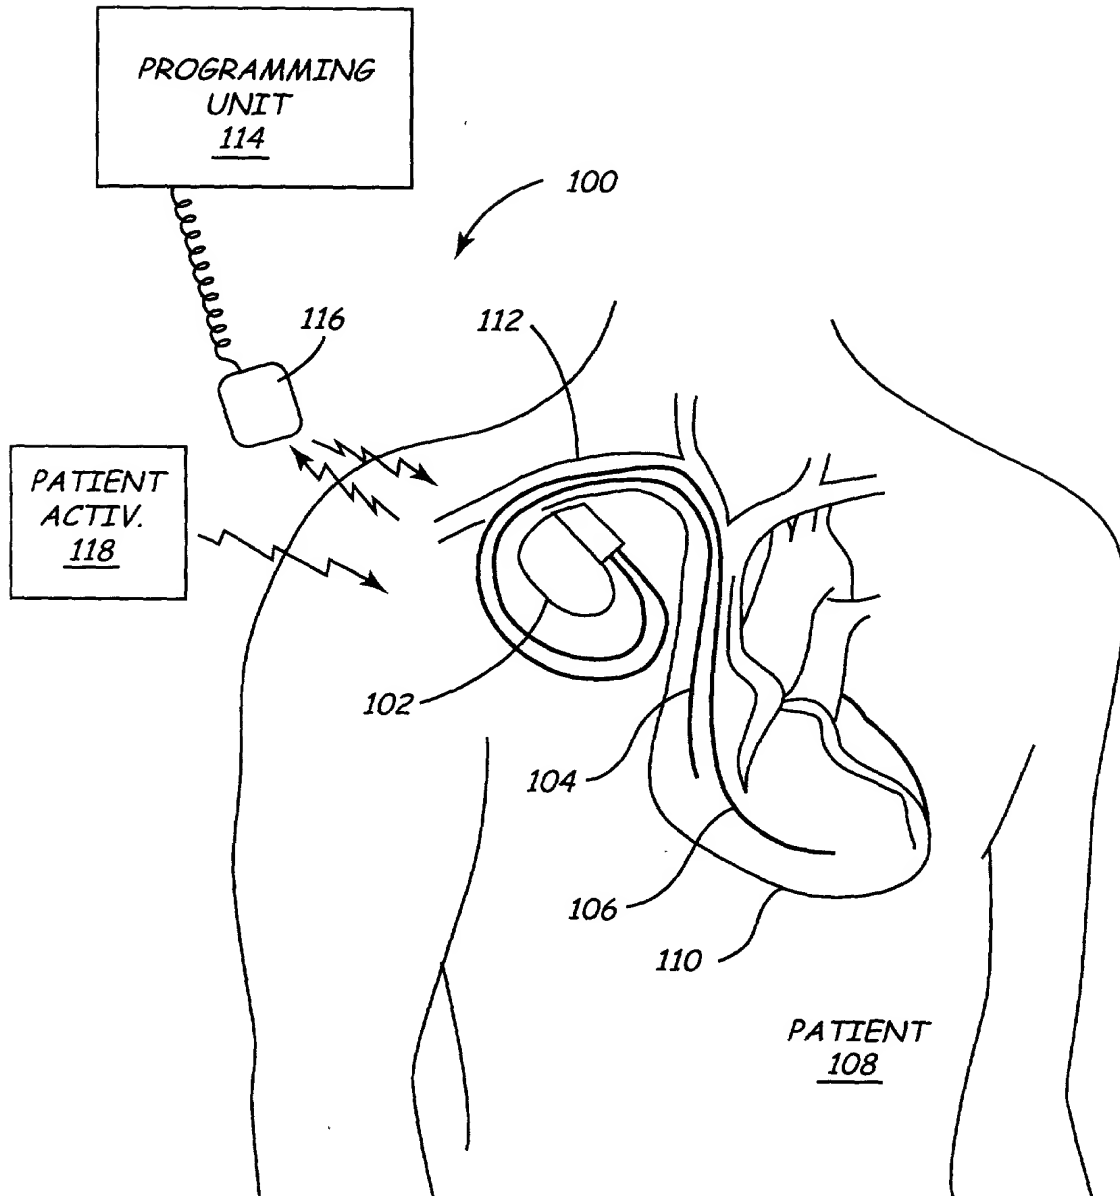


1/21



**FIG. 1**

2/21

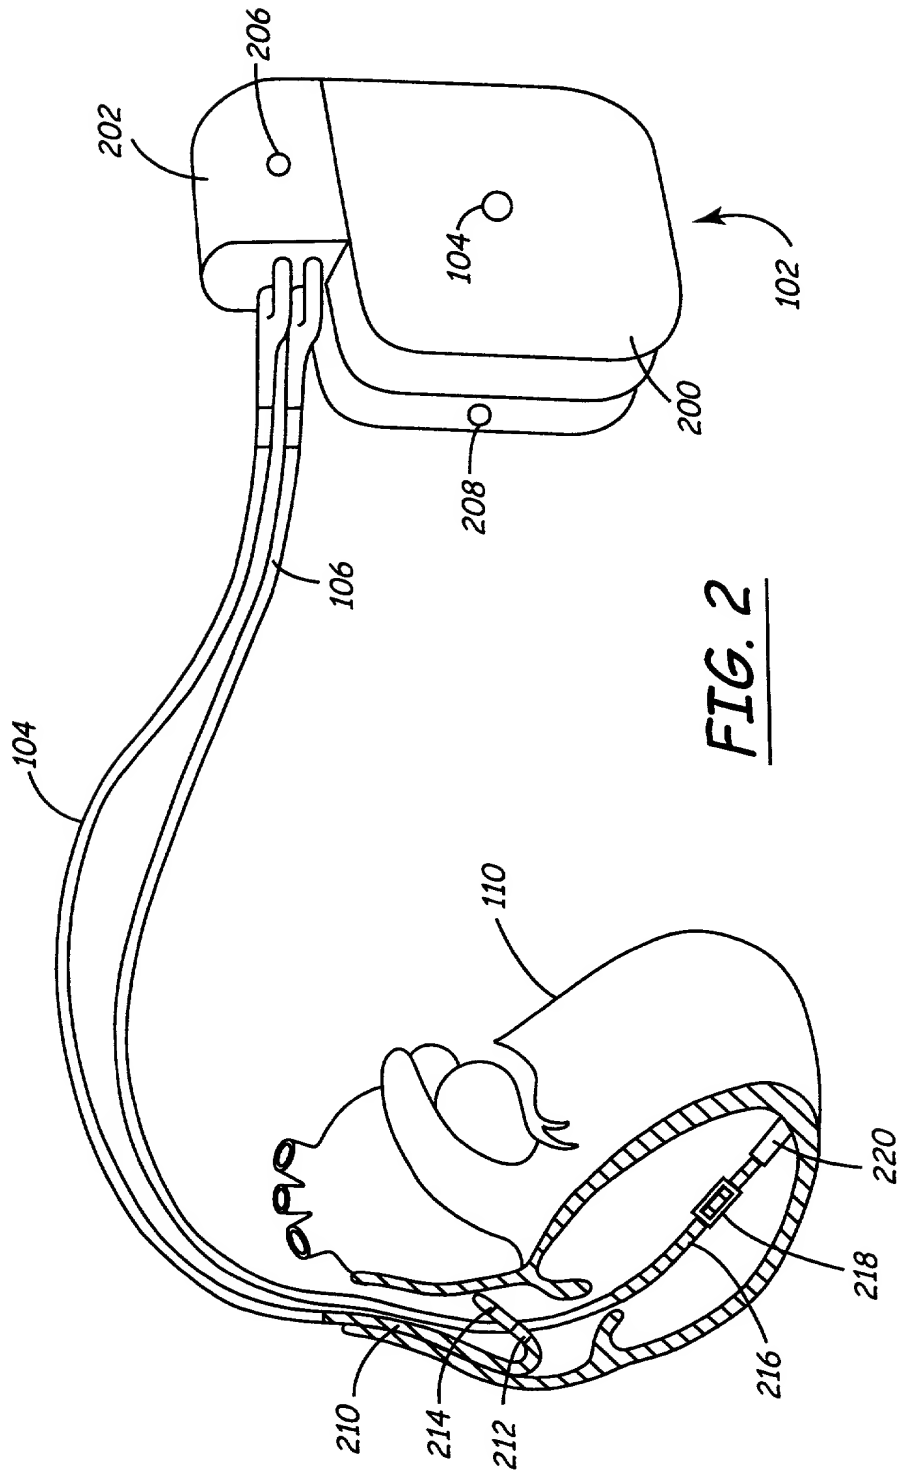

3/21

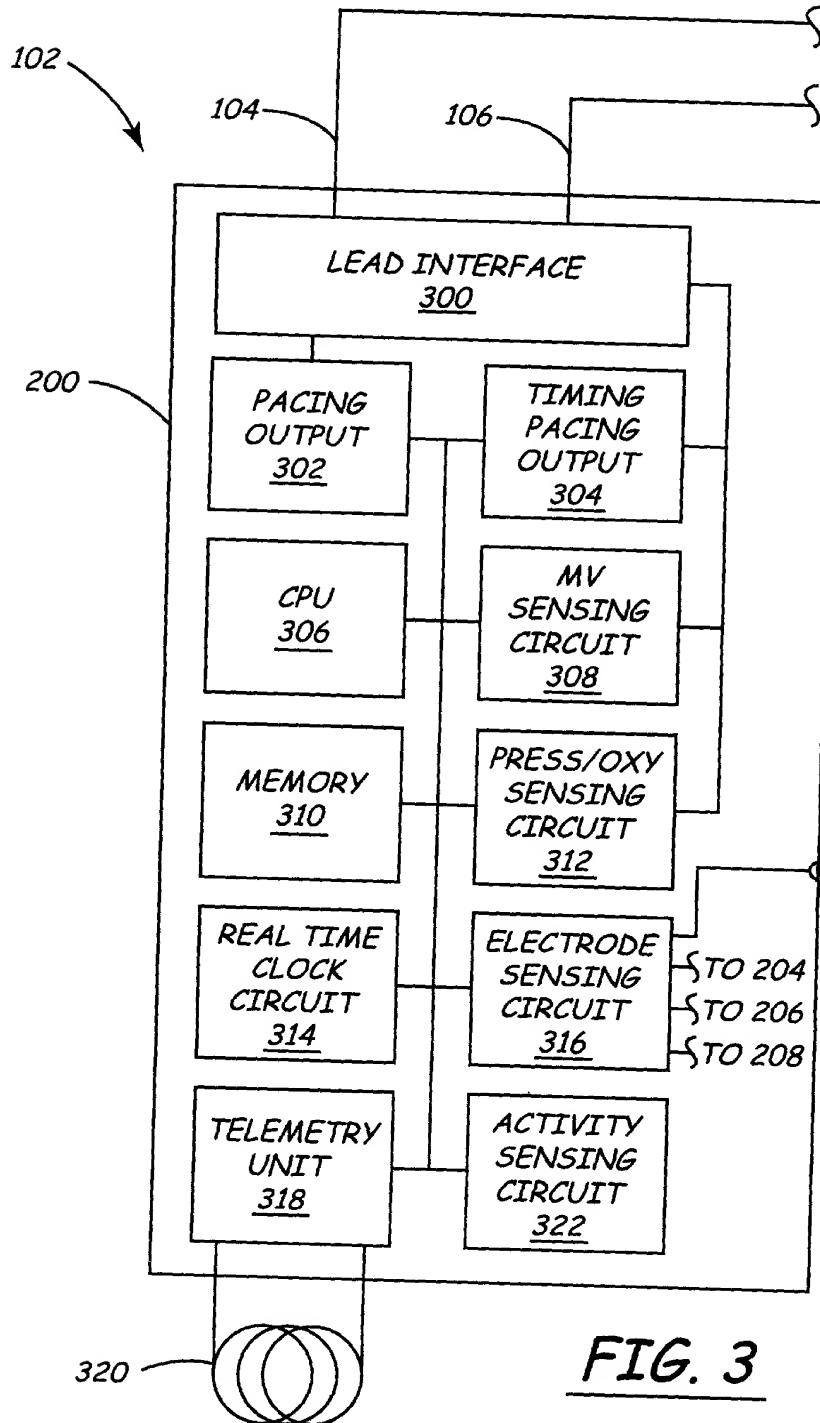


FIG. 3

0945195 3/21/04

4/21

*MEMORY 310*

*OPERATING MODE VALUE 400*

*HIGH RATE LIMIT VALUE 402*

*TRANSFER FUNCTION VALUE(S) 404*

*RATE RESPONSE SOFTWARE 406*

*FIG. 4*

5/21

*TIMING/PACING CONTROL 304*

*DEMAND MODE VALUE 500*

*LOW RATE LIMIT VALUE 502*

*A-V INTERVAL VALUE 504*

*FIG. 5*

6/21

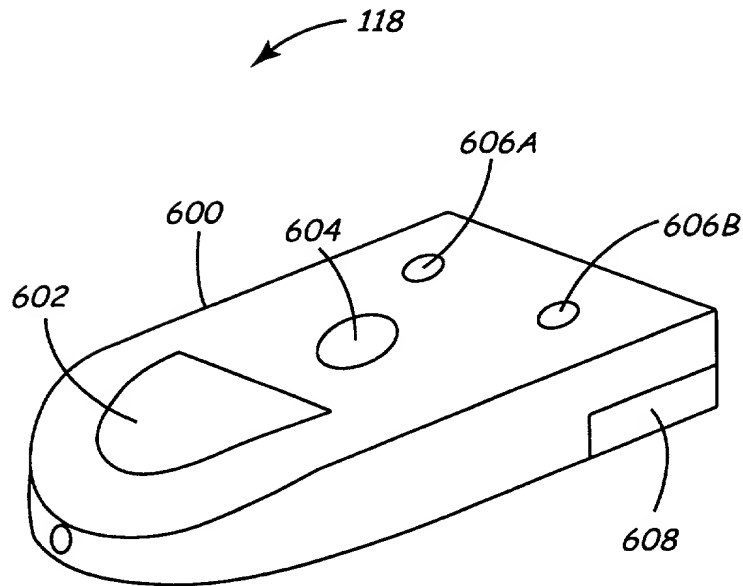


FIG. 6

7/21

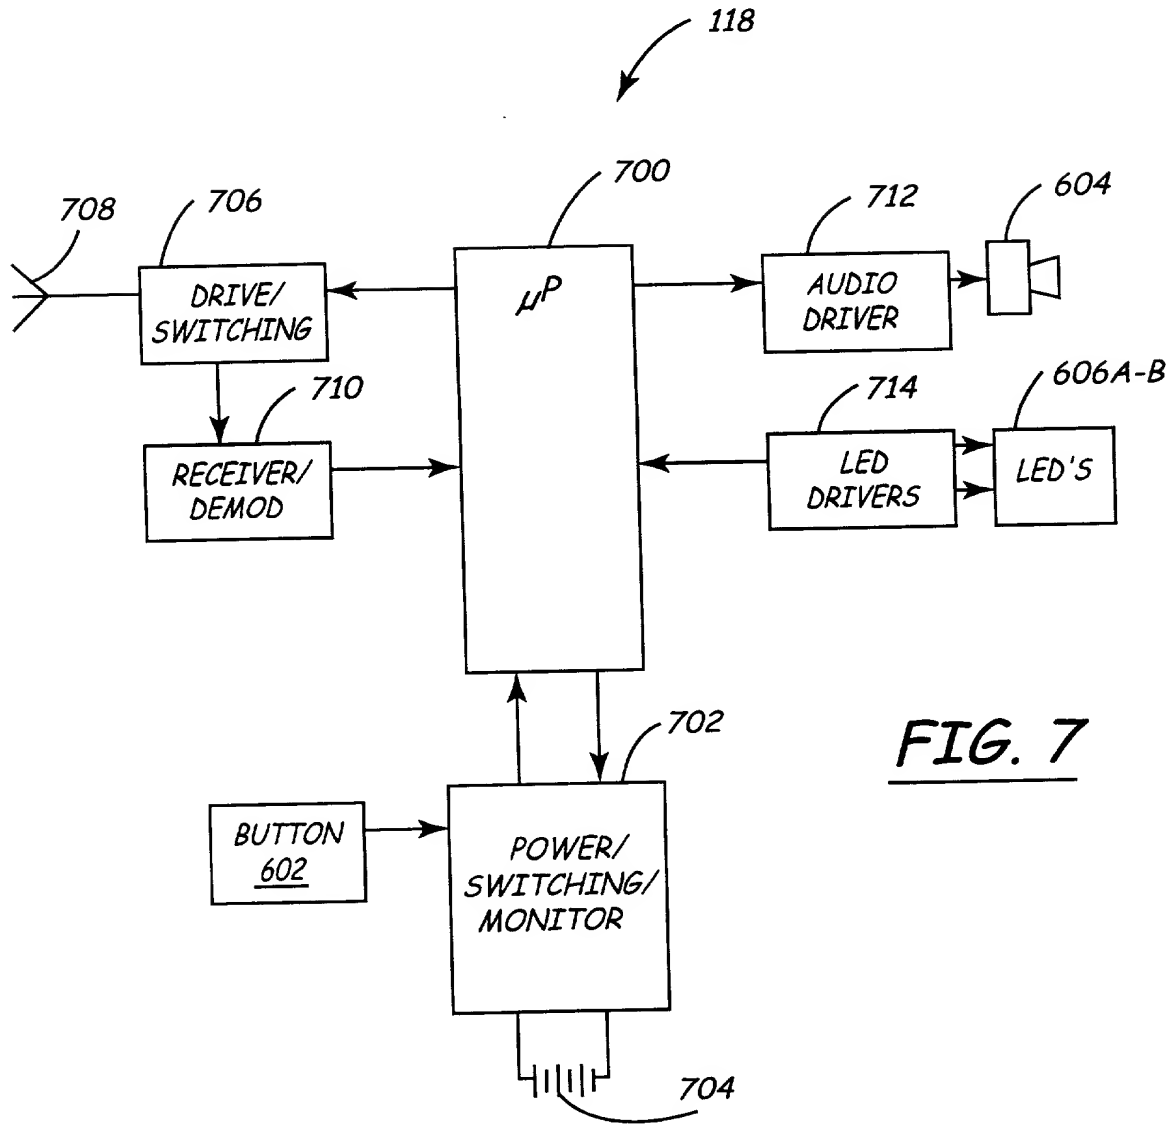


FIG. 7

8/21

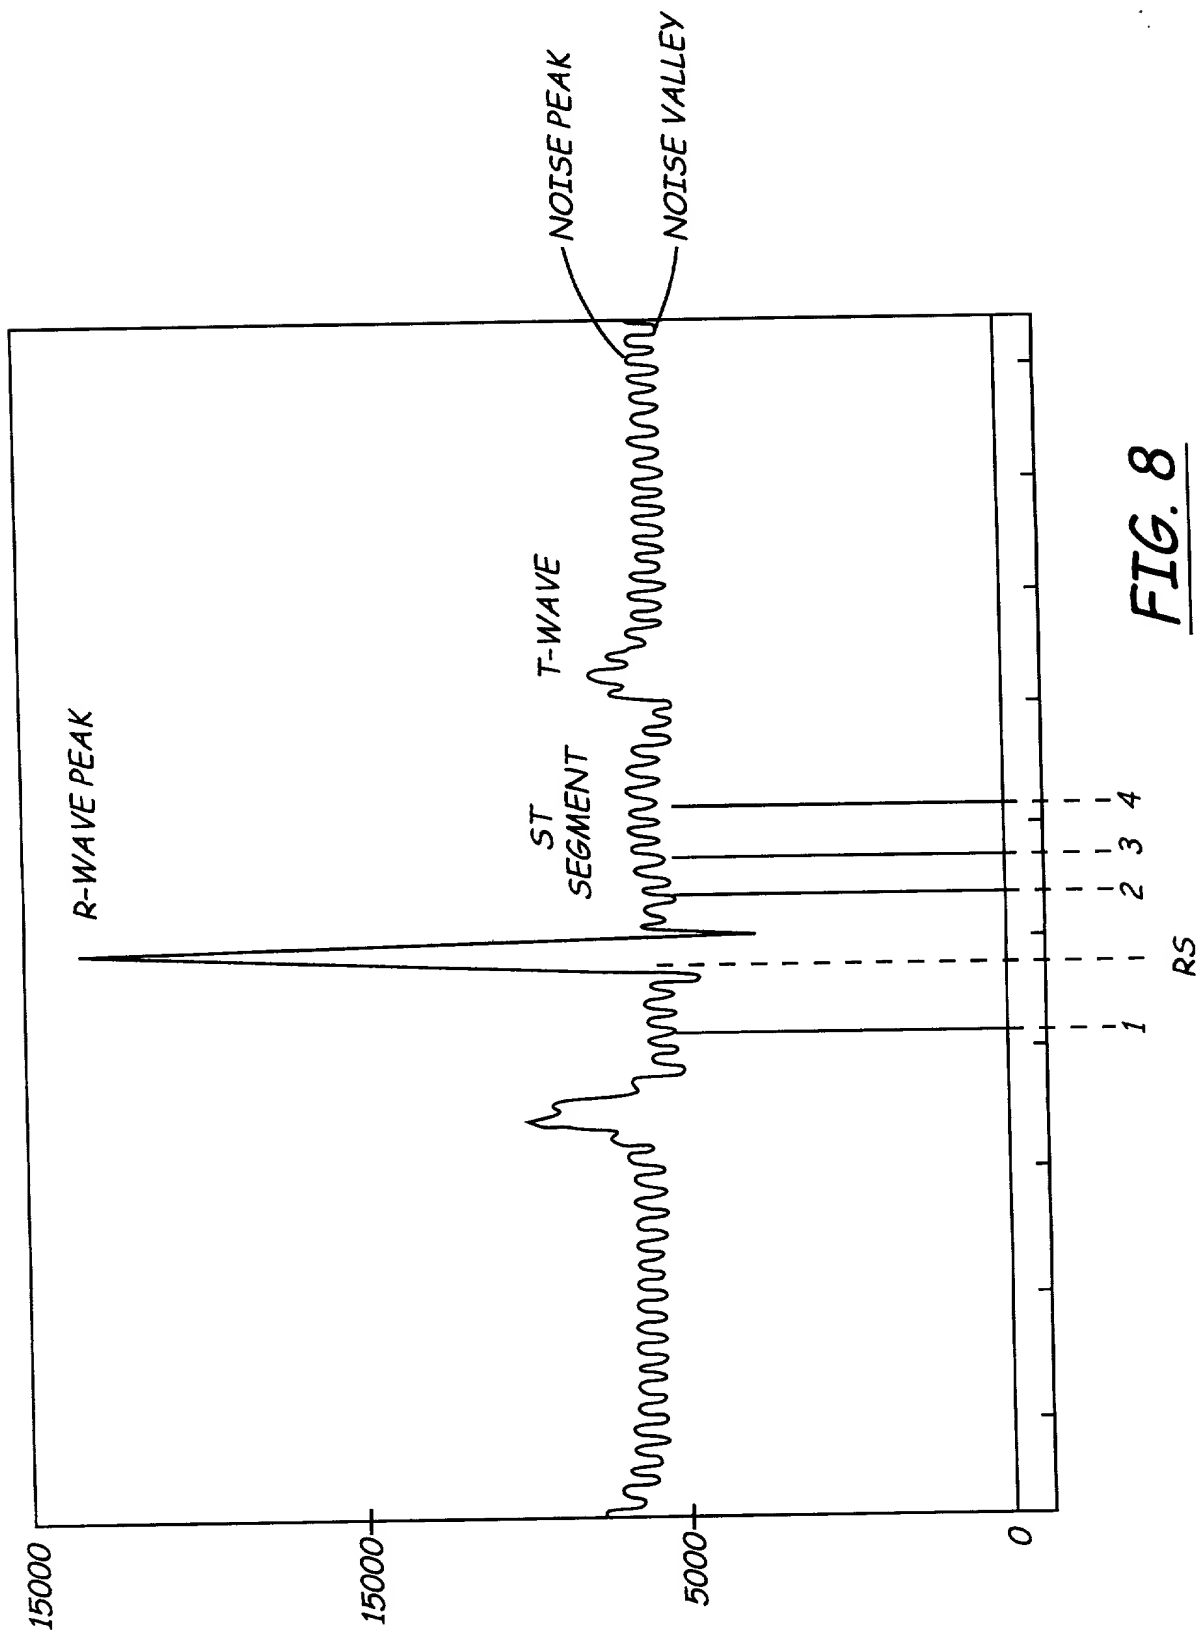


FIG. 8

FIG. 8 "50 F 54650"



9/21

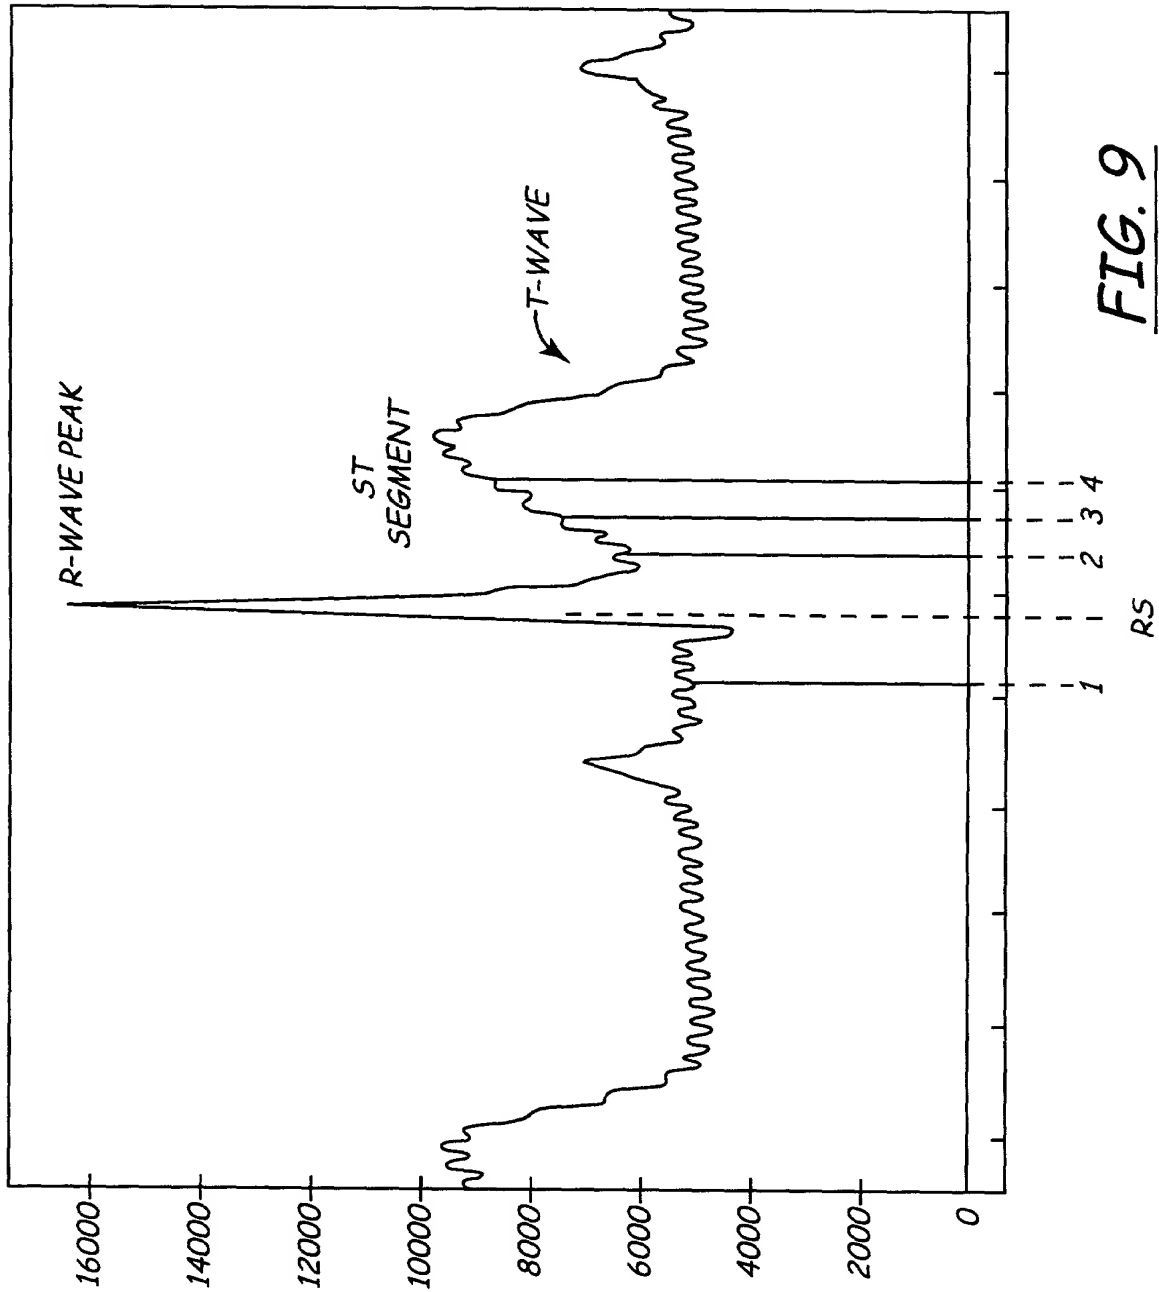


FIG. 9

10/21

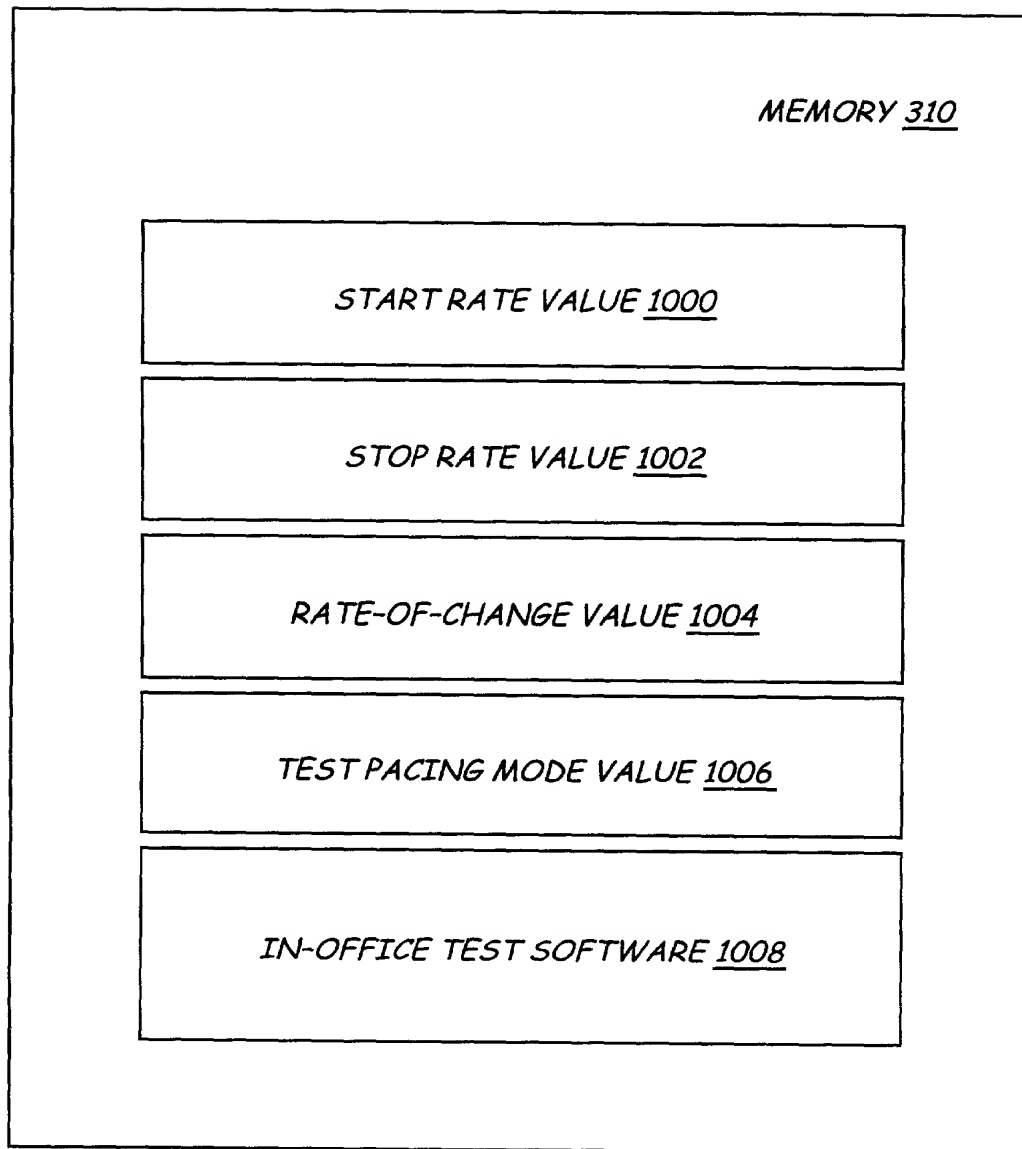


FIG. 10

11/21


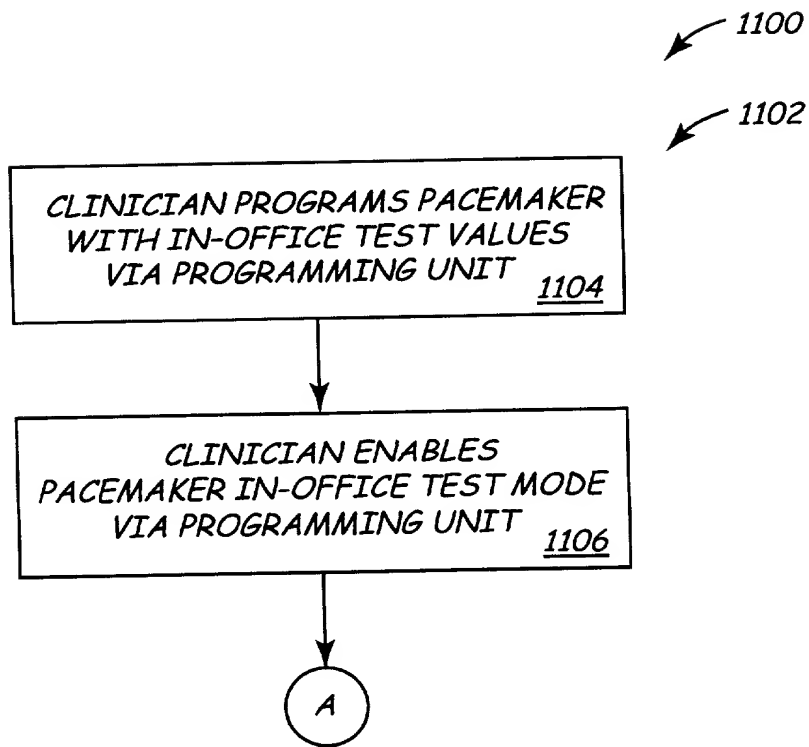


FIG. 11A

12/21

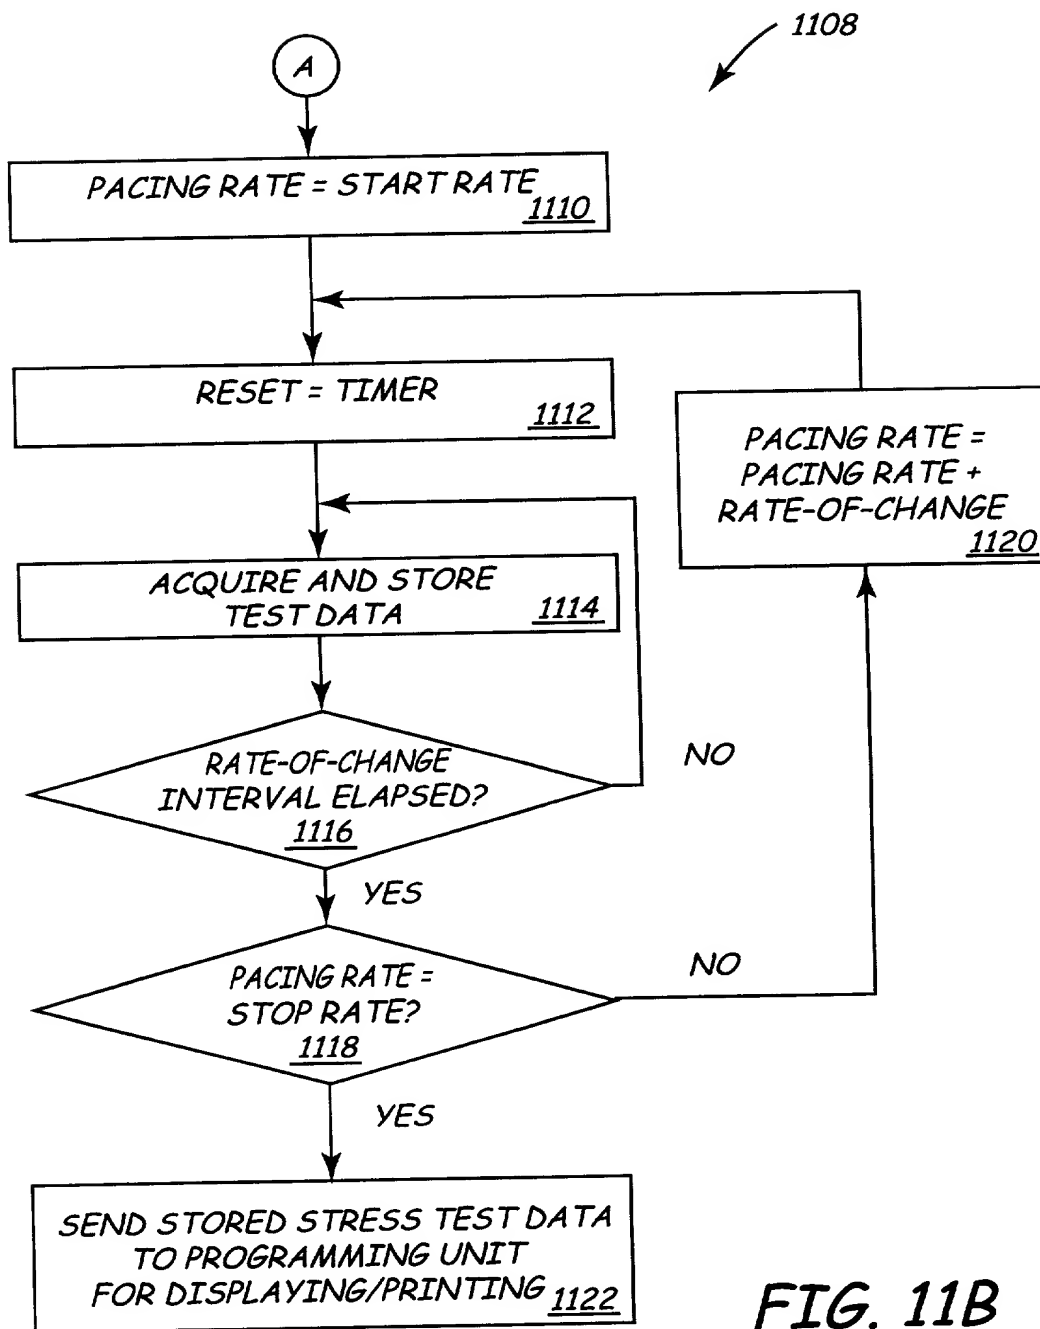

13/21

MEMORY 310

TEST FREQUENCY VALUE 1200

TEST START TIME VALUE 1202

START RATE VALUE 1204

STOP RATE VALUE 1206

RATE-OF-CHANGE VALUE 1208

TEST PACING MODE VALUE 1210

ABORT PARAMETERS 1211

AMBULATORY STRESS TEST  
SOFTWARE 1212

FIG. 12

14/21

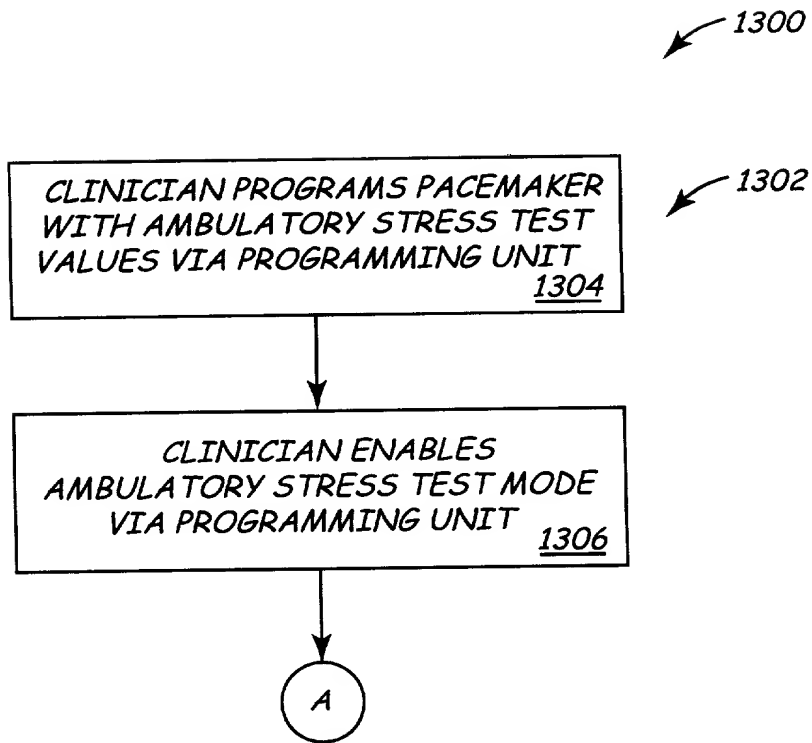


FIG. 13A

15/21

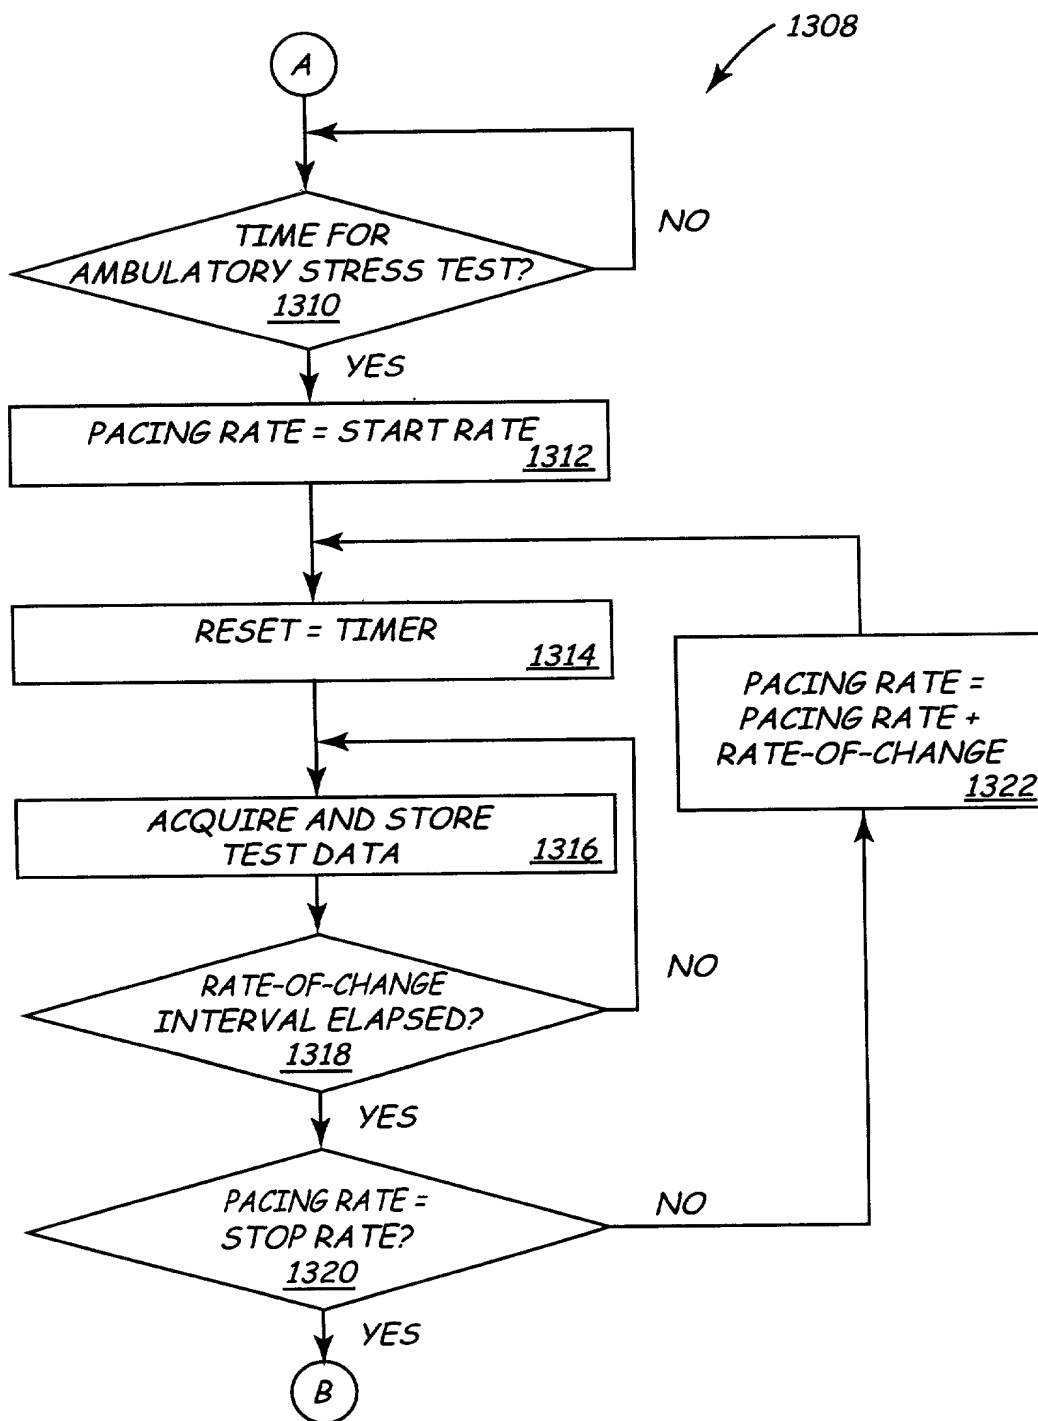


FIG. 13B

16/21

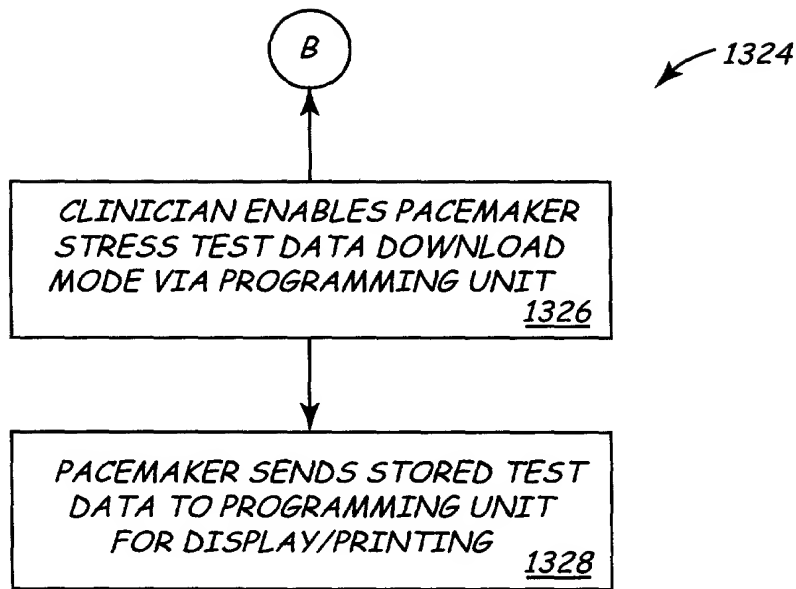


FIG. 13C



17/21

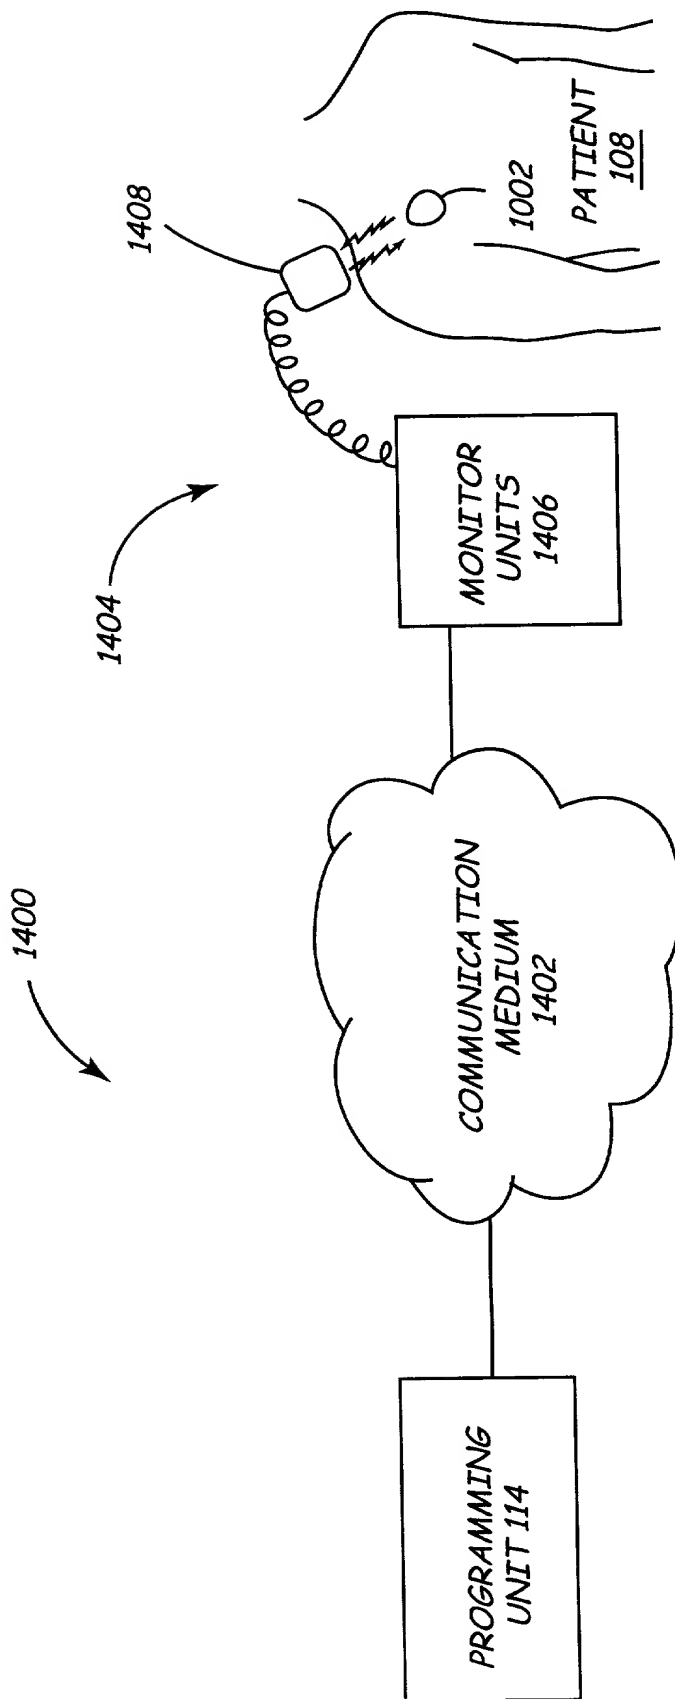


FIG. 14

PROGRAMMING UNIT 114



FIG. 15

19/21

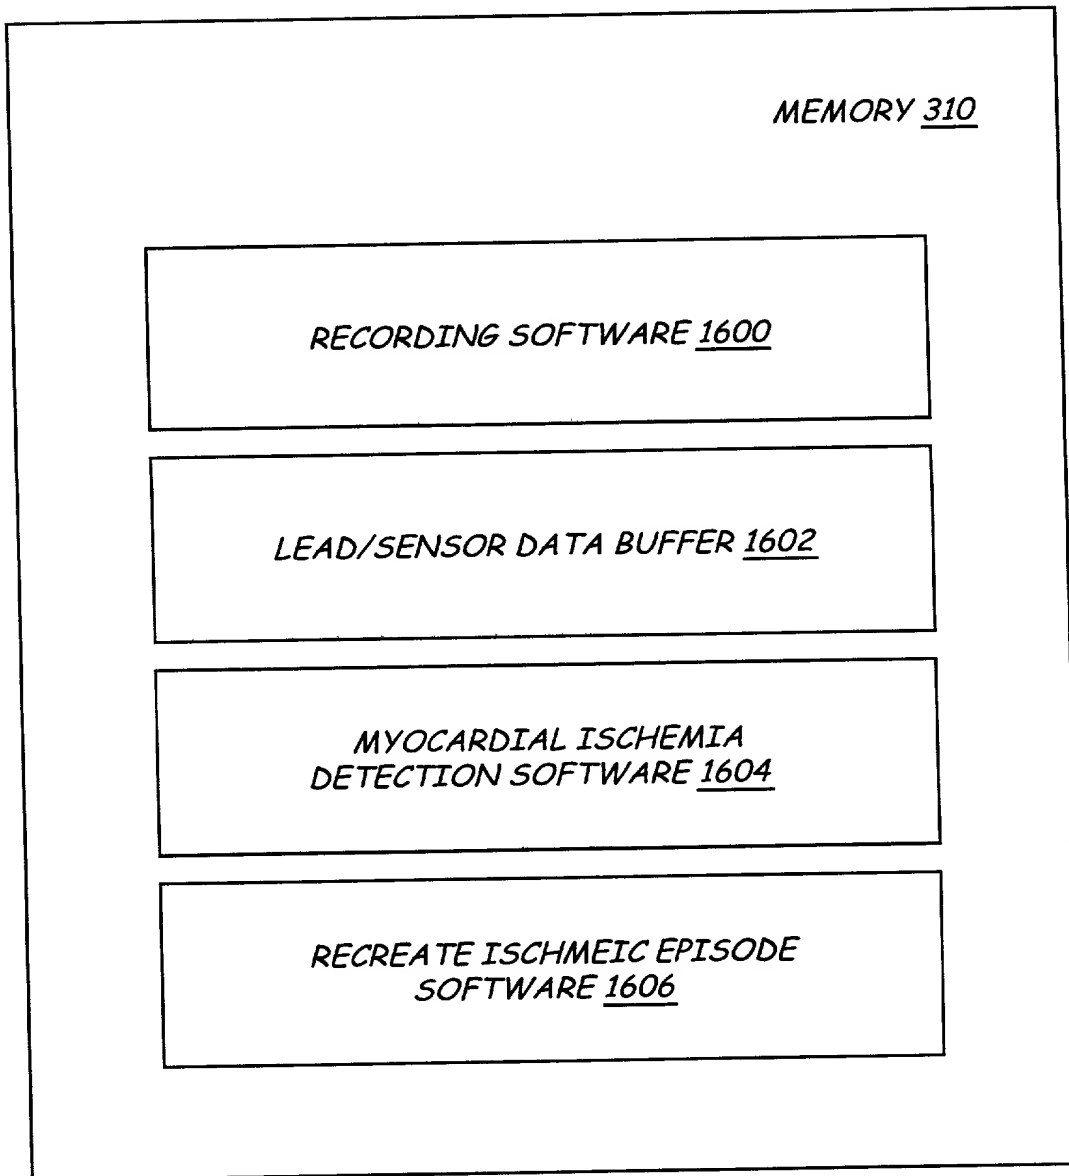


FIG. 16

20/21

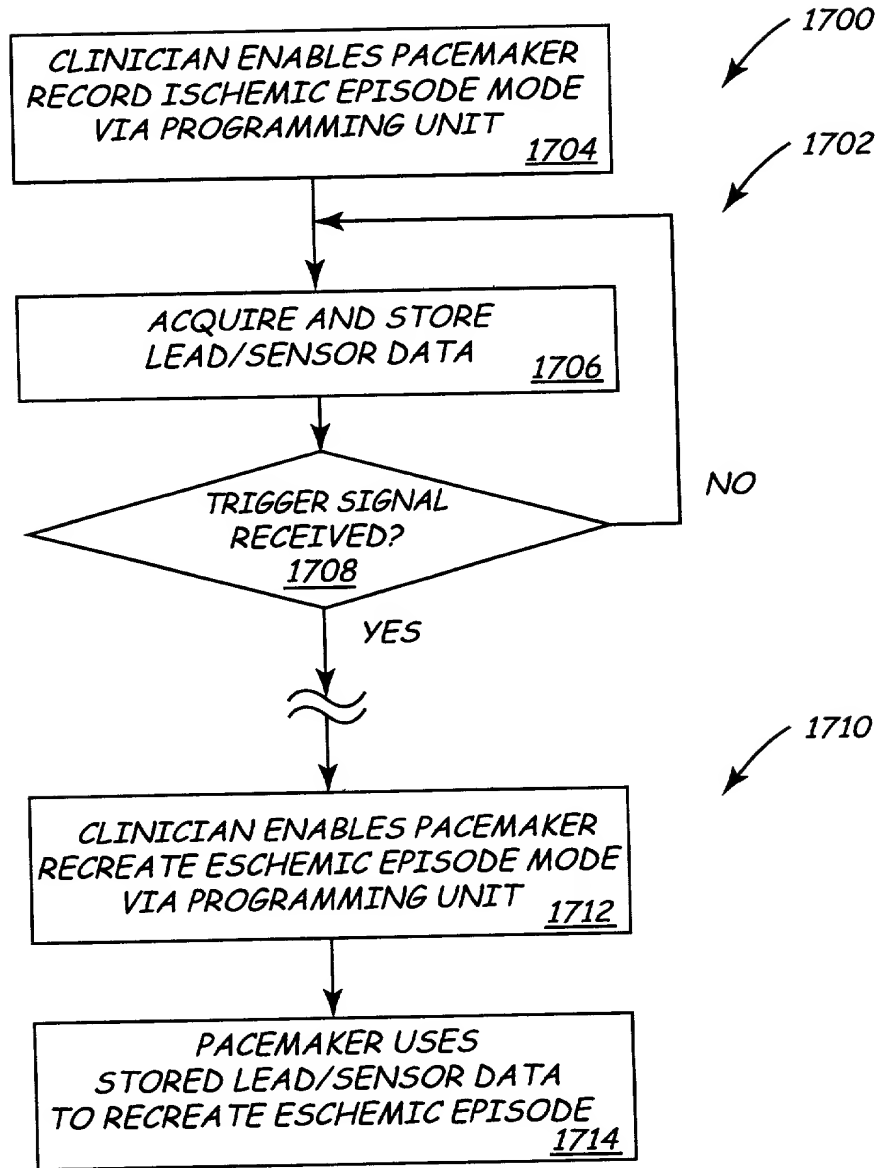


FIG. 17

21/21

PROGRAMMING UNIT 114

1500

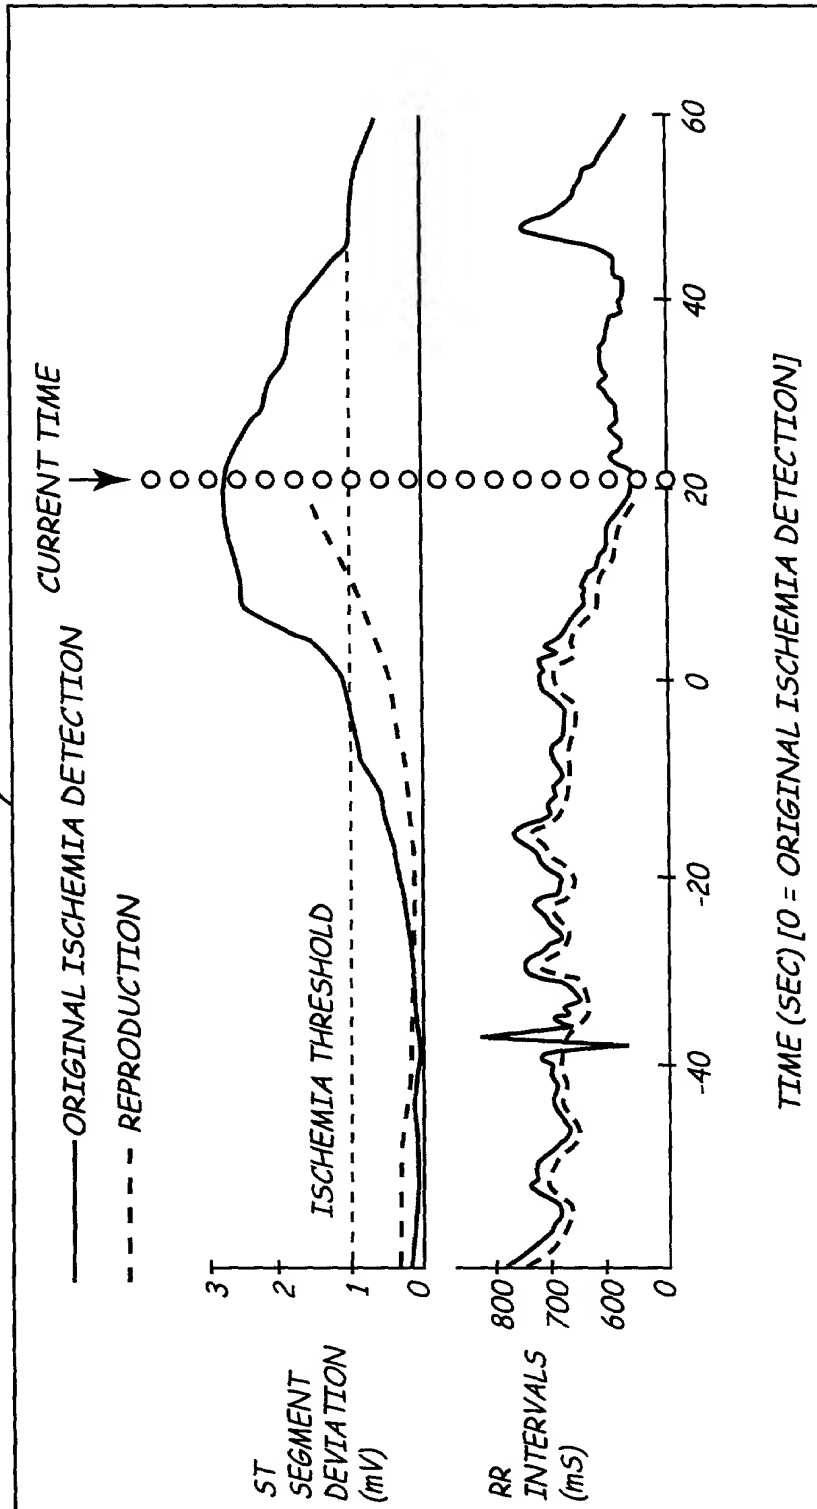


FIG. 18